



H0081_ X20 Standard Configuration 093014


Cytometer:	LSRFortessa	User:	corestaff
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	5/31/2018 2:03:22 PM
Window Extension:	10.00		

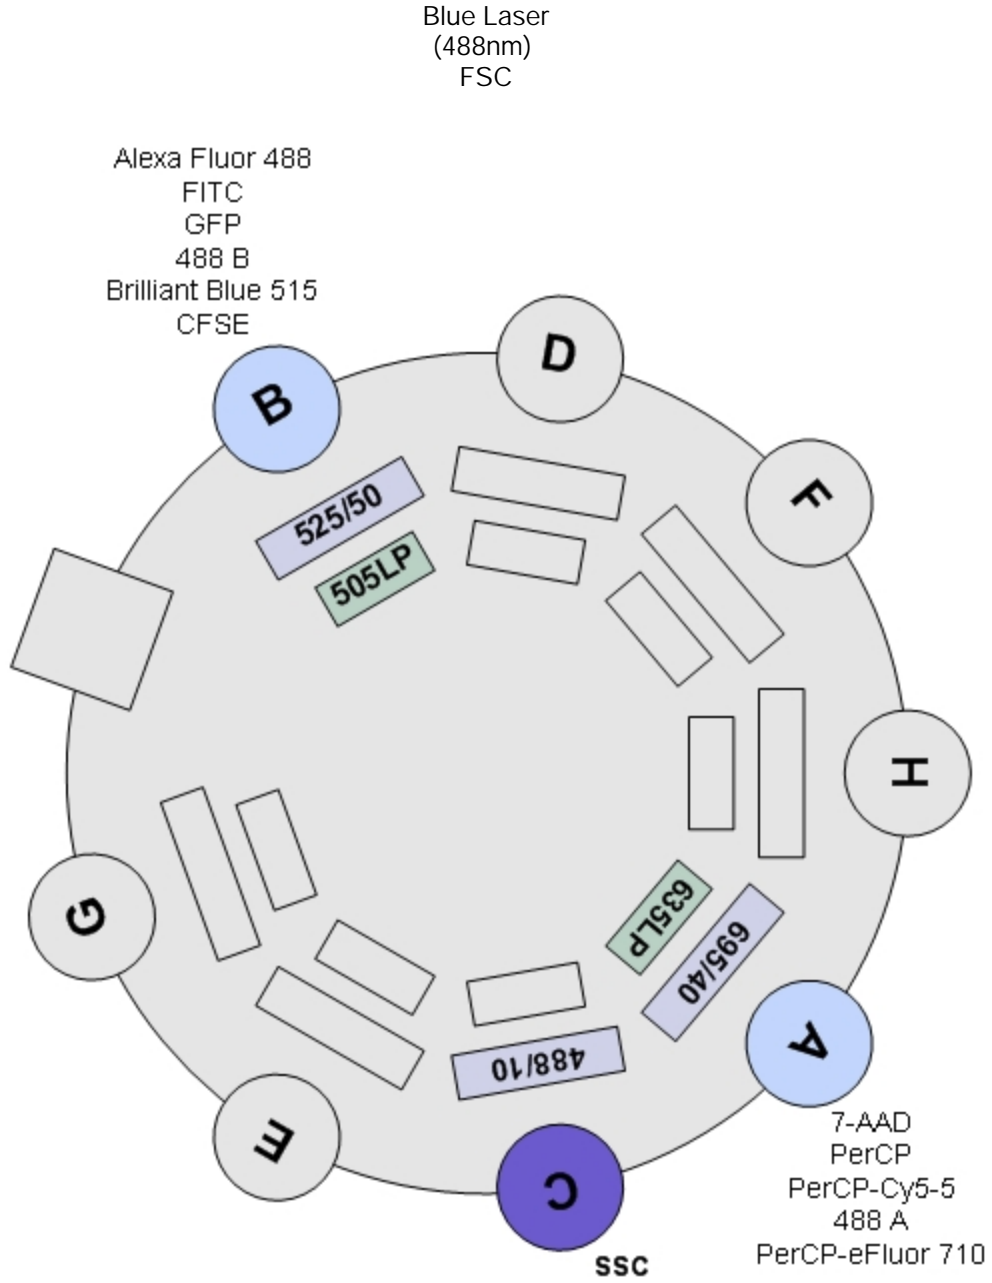

Violet Laser
(405nm)

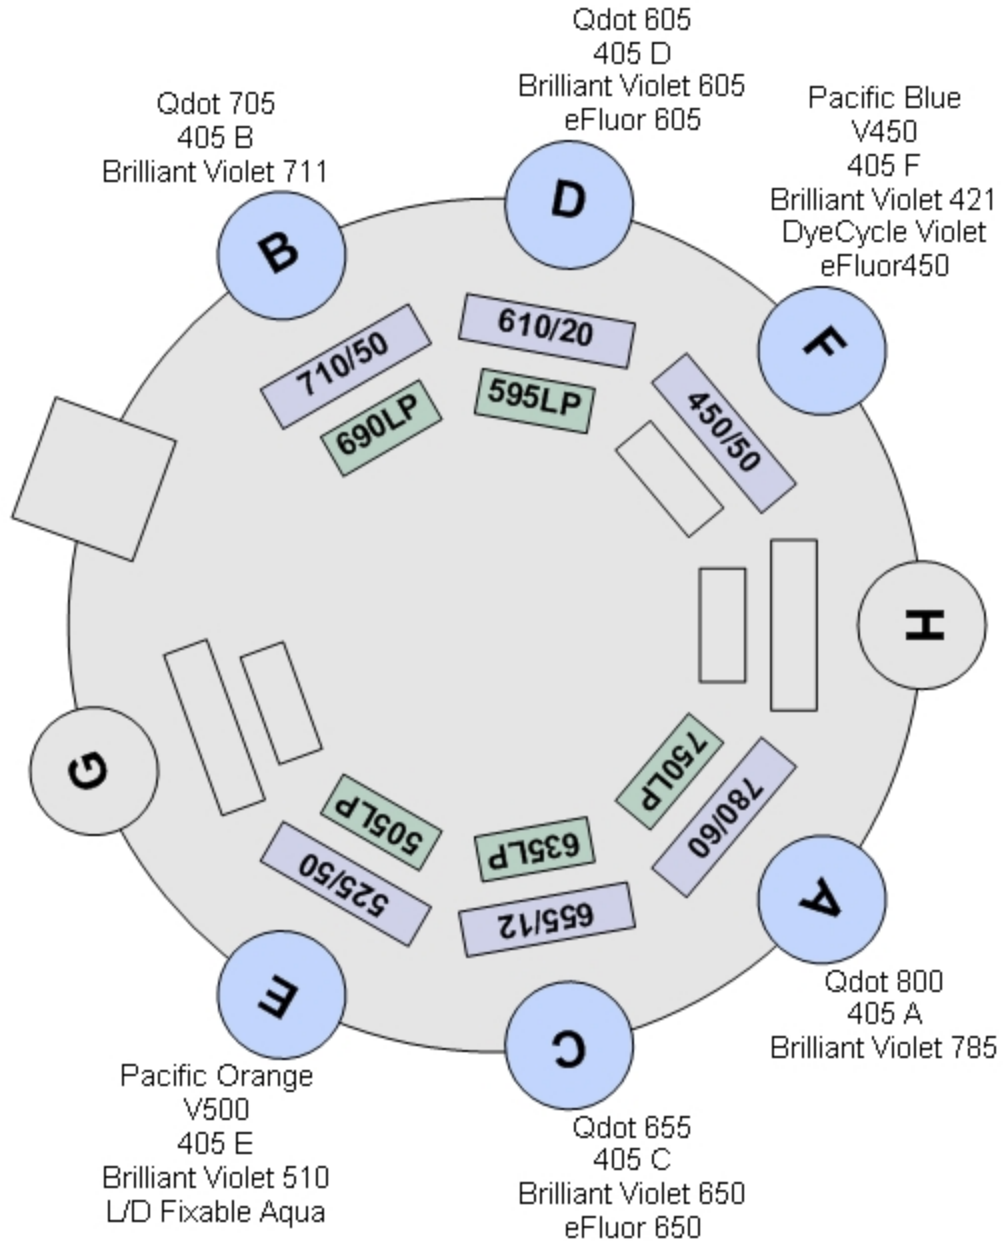


Red Laser
(640nm)

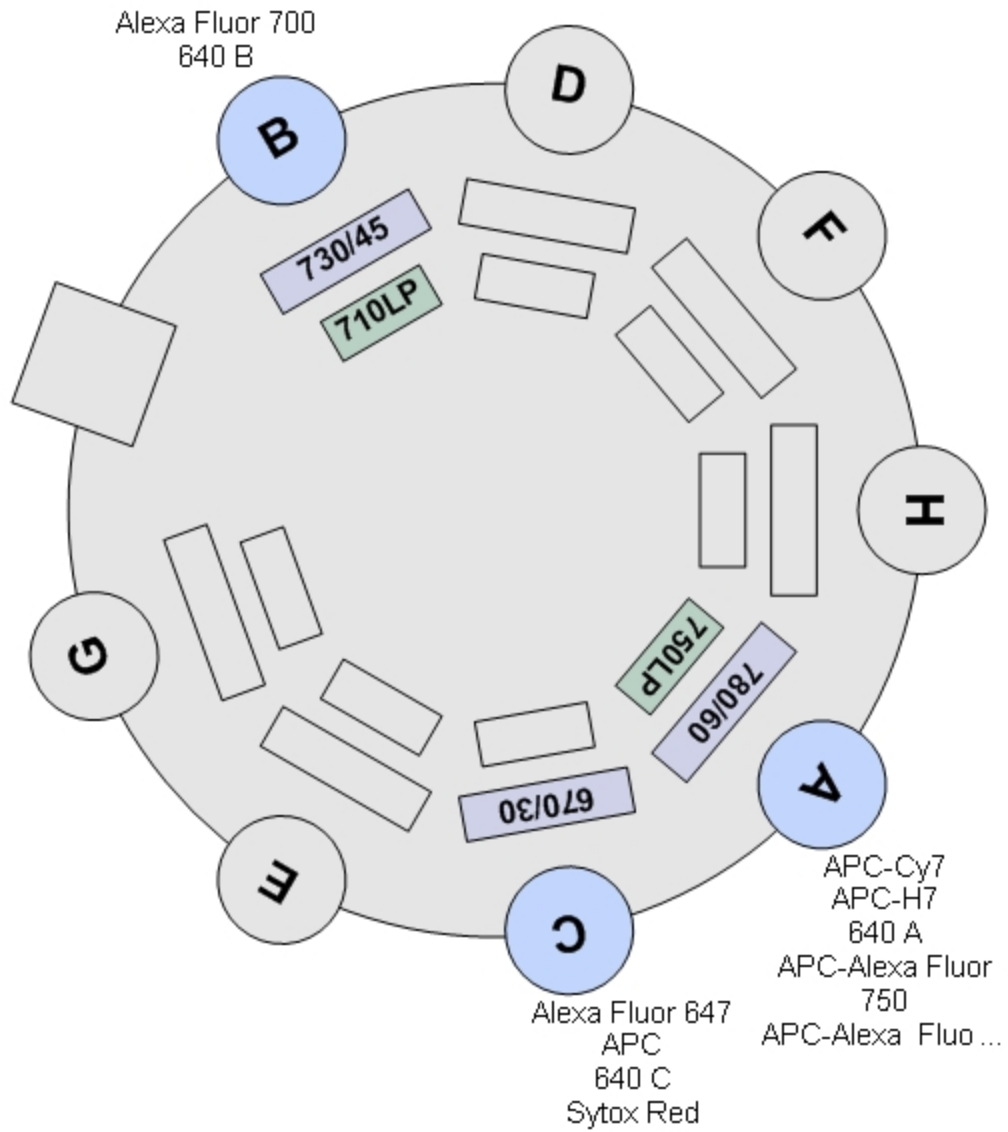


Yellow Green Laser
(561nm)

PE-CF594
PE-Texas Red
561 B
mCherry
PE-Alexa Fluor
610

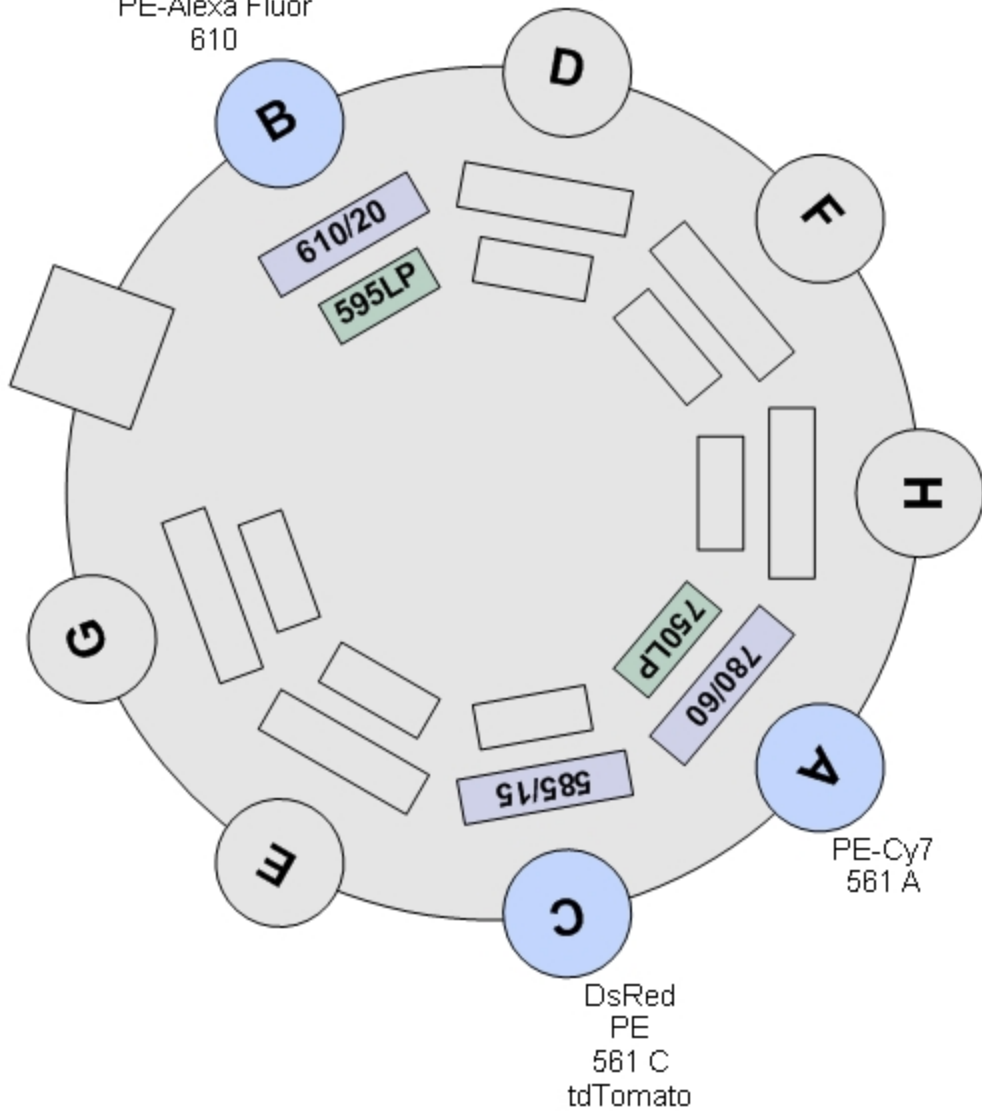

UV Laser
(355nm)

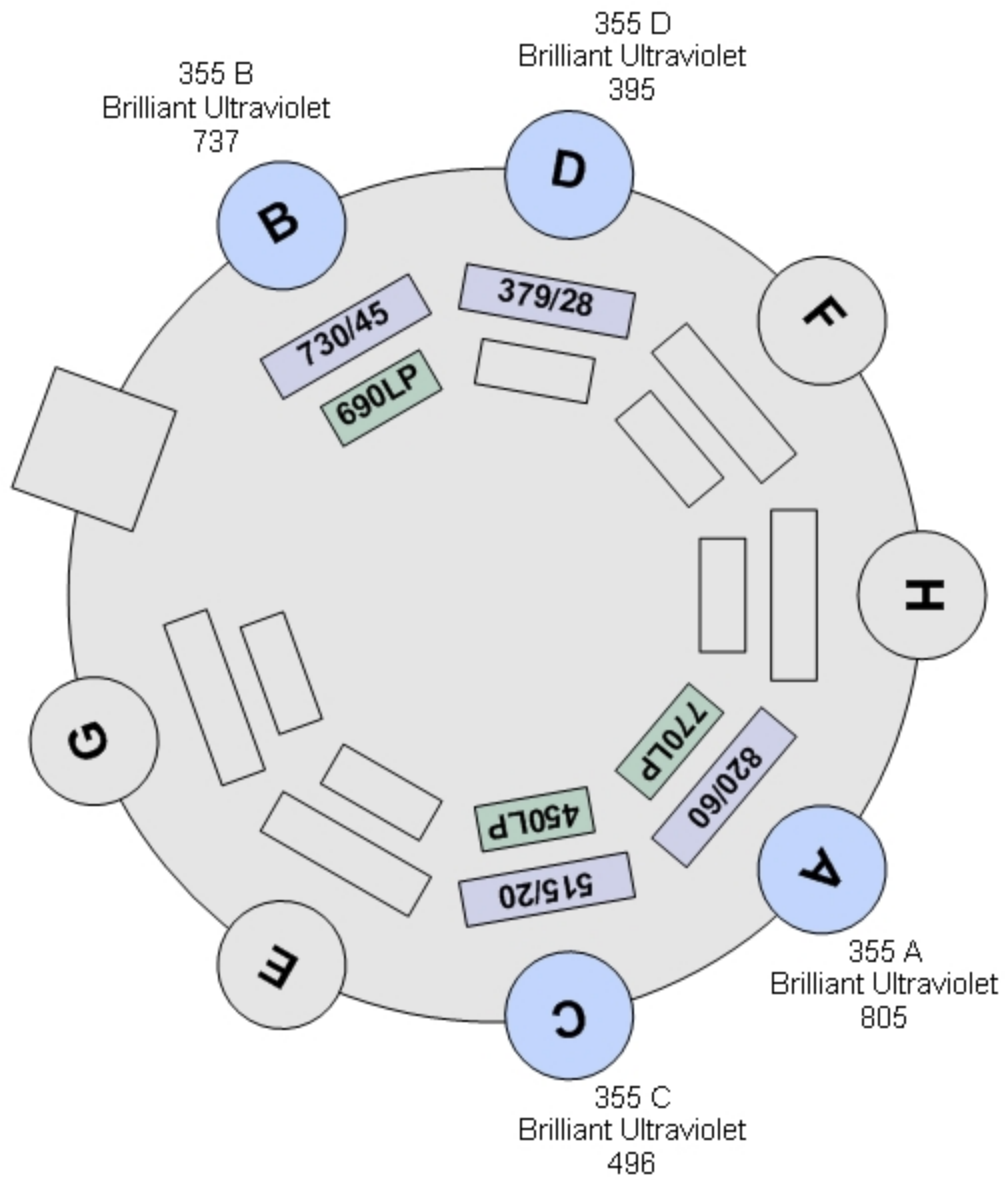

Comments: