





# H1010 Standard Configuration 100813

Cytometer:	LSRII	User:	farrarlab
Cytometer Name:	LSRII	Institution:	
Serial Number:	10100002	Software:	BD FACSDiva 6.2
Input Device:	Manual	Date:	10/15/2013 10:28:40 AM
Window Extension:	10.00		

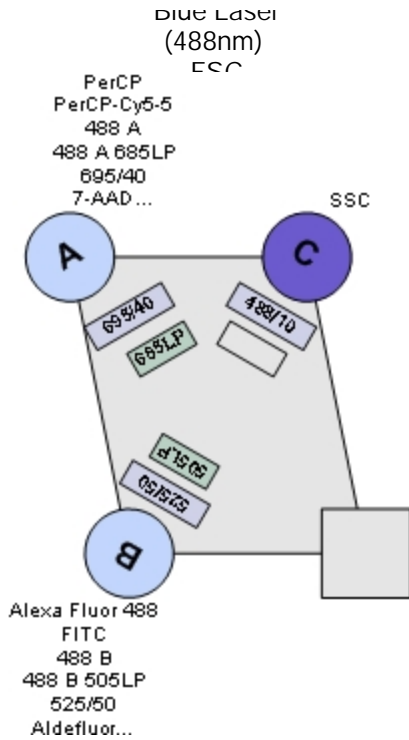

Violet Laser  
(405nm)

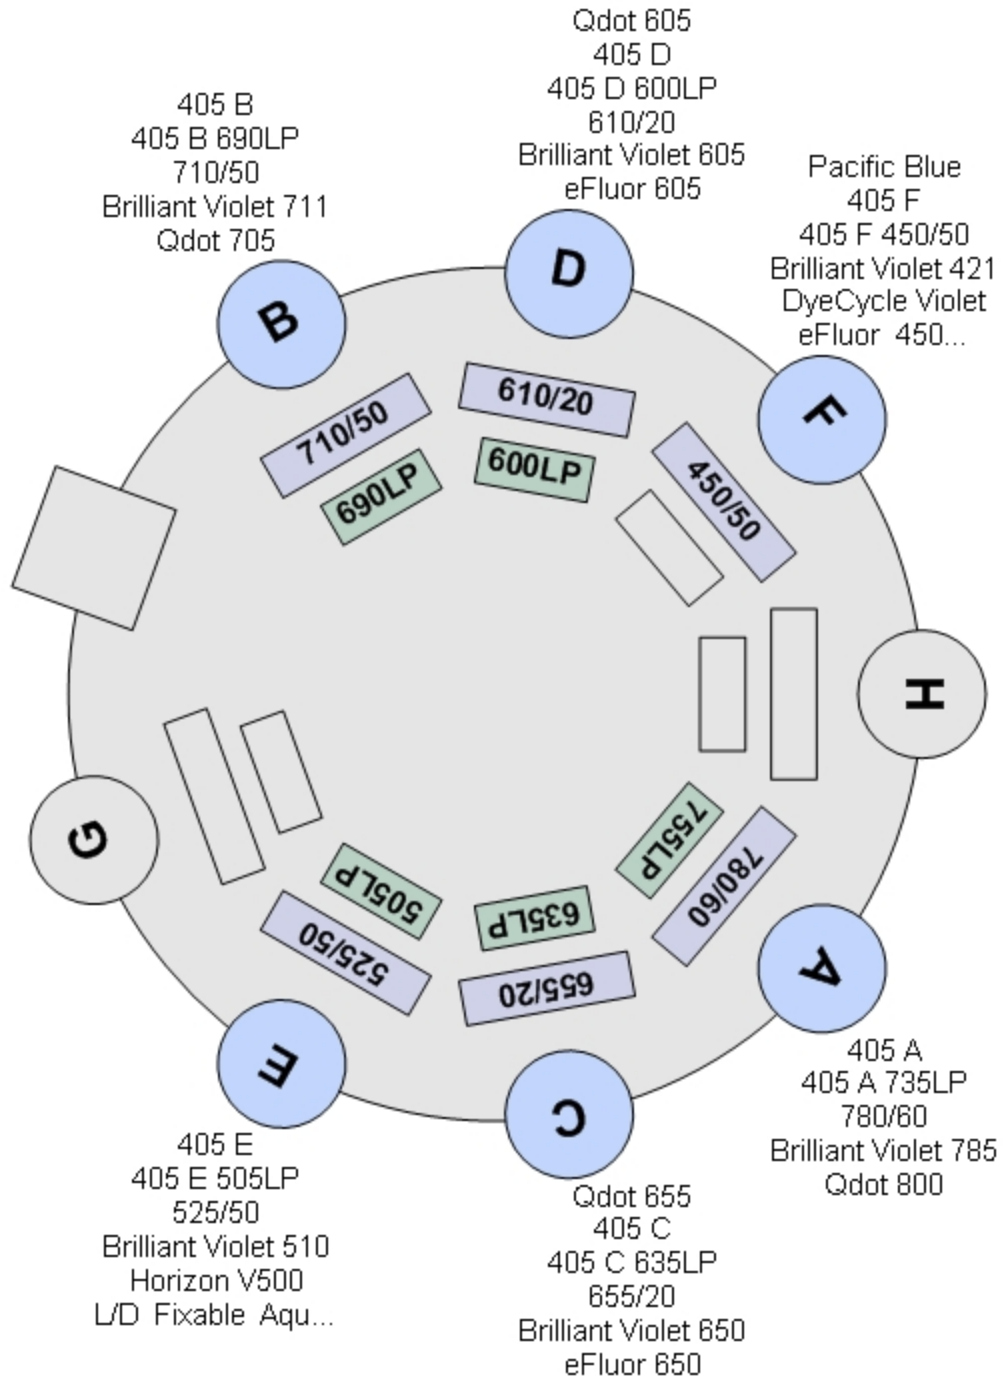

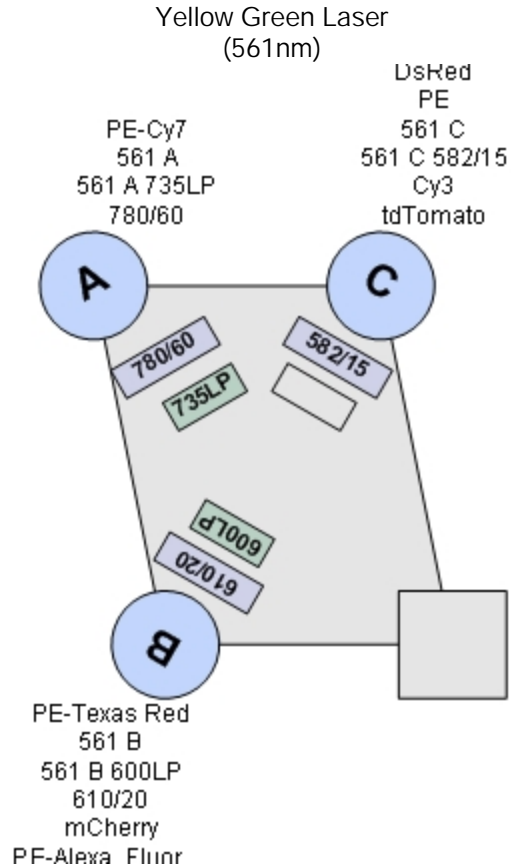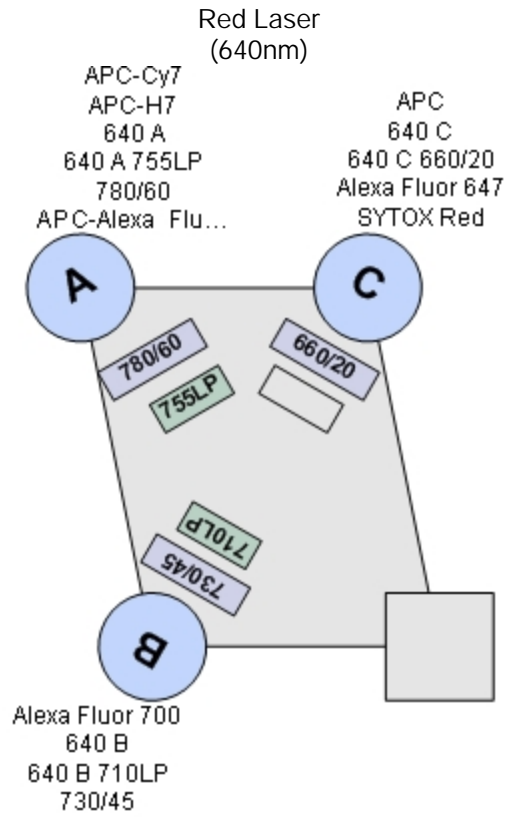

Comments: