



LSRFortessa H1770 Standard Configuration


Cytometer:	LSRII	User:	corestaff
Cytometer Name:	LSRII	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0
Input Device:	Manual	Date:	6/17/2015 11:08:53 AM
Window Extension:	10.00		

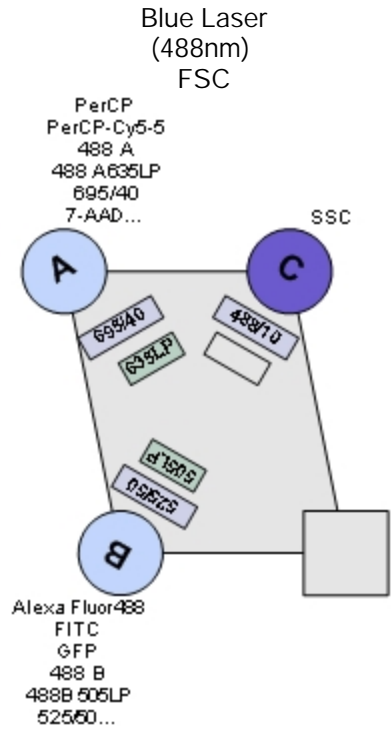


Violet Laser
(405nm)

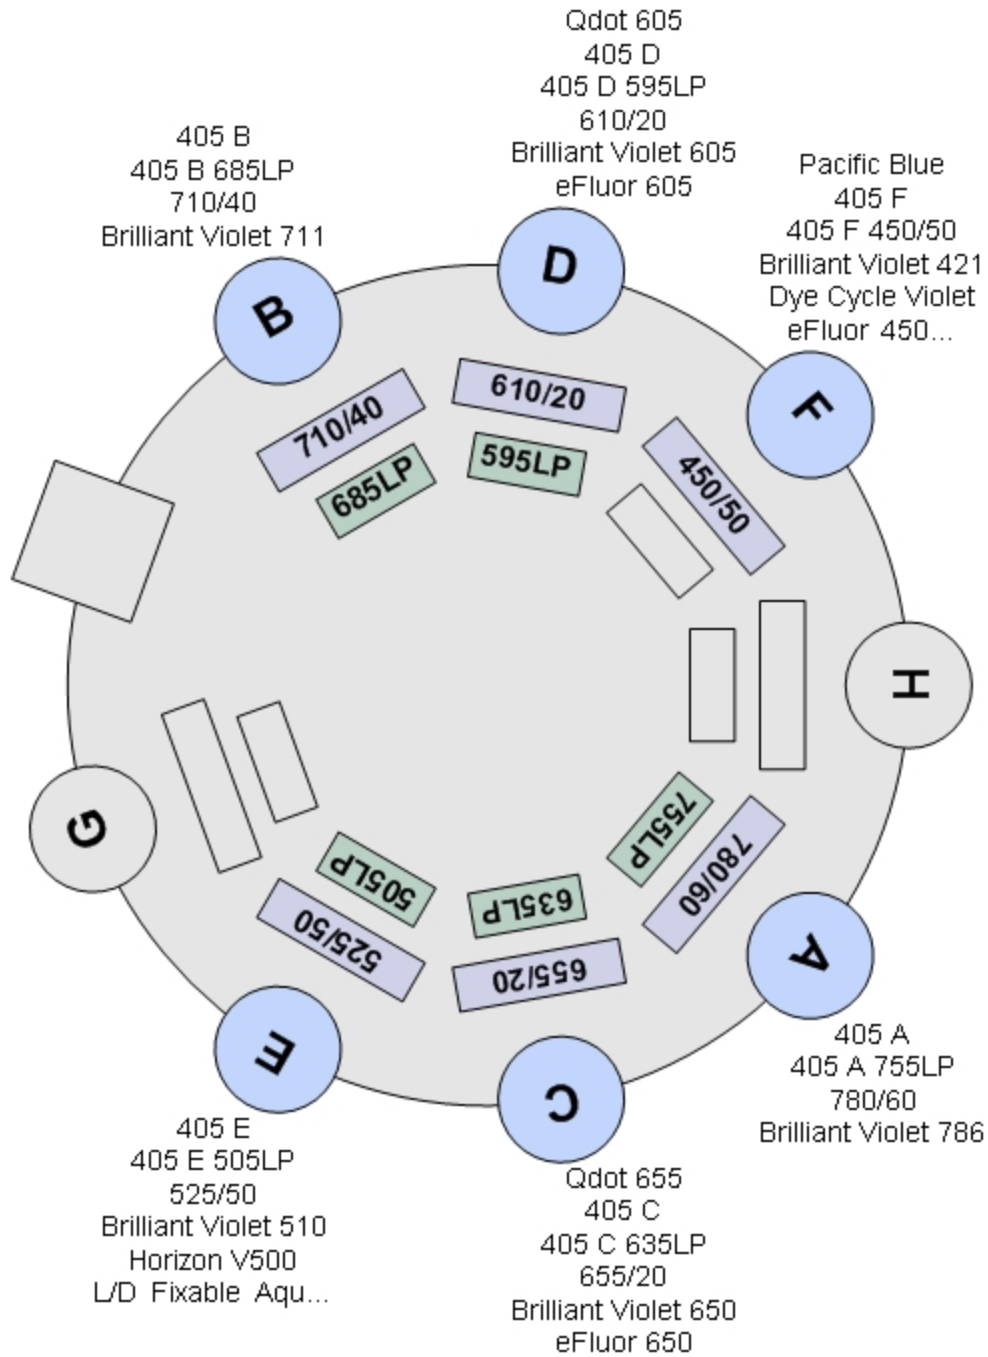


Red Laser
(640nm)

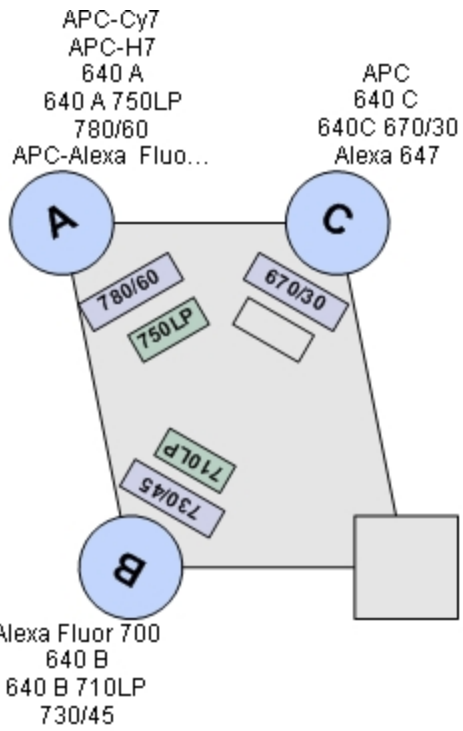

UV Laser
(355nm)

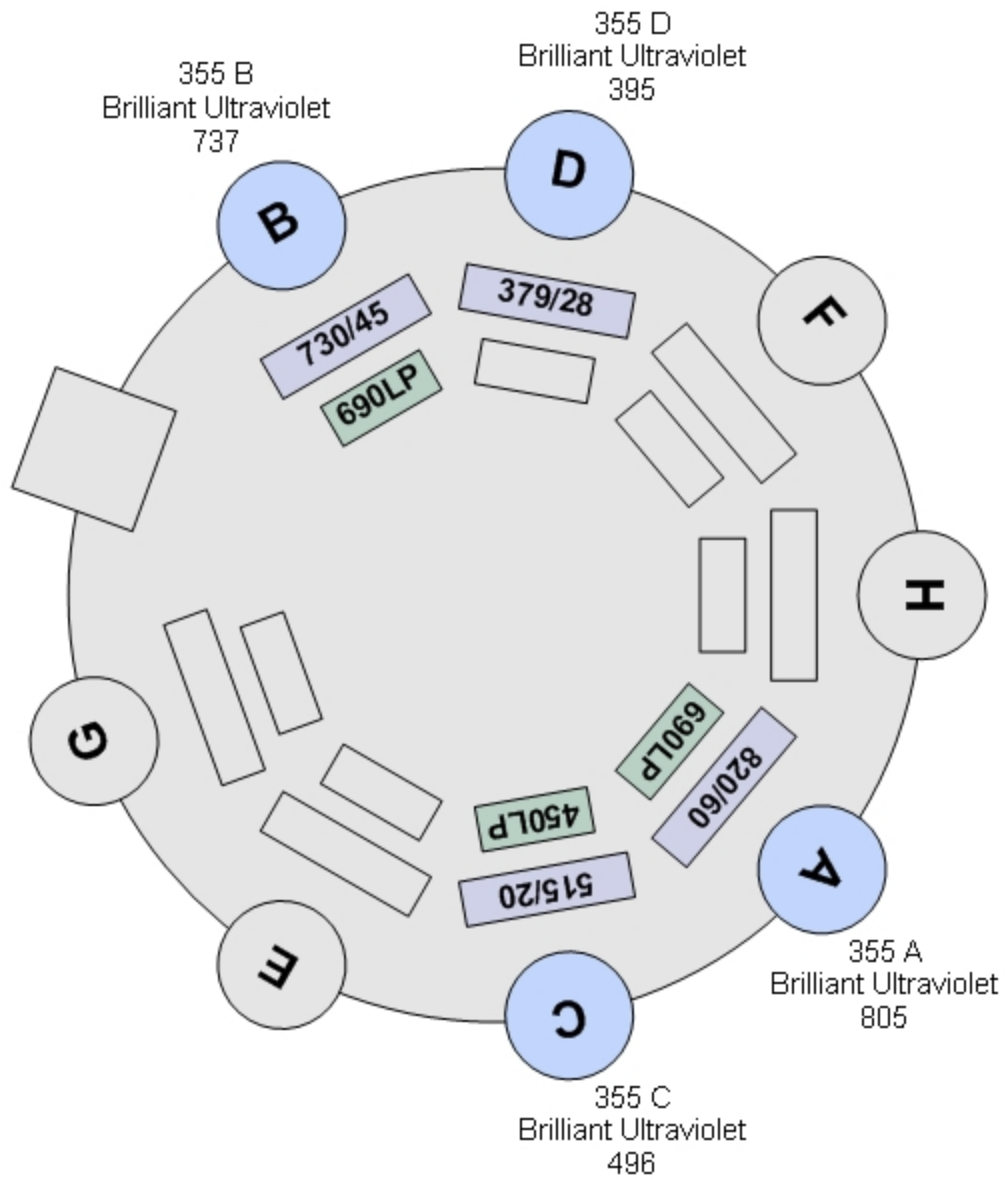

YG Laser
(561nm)

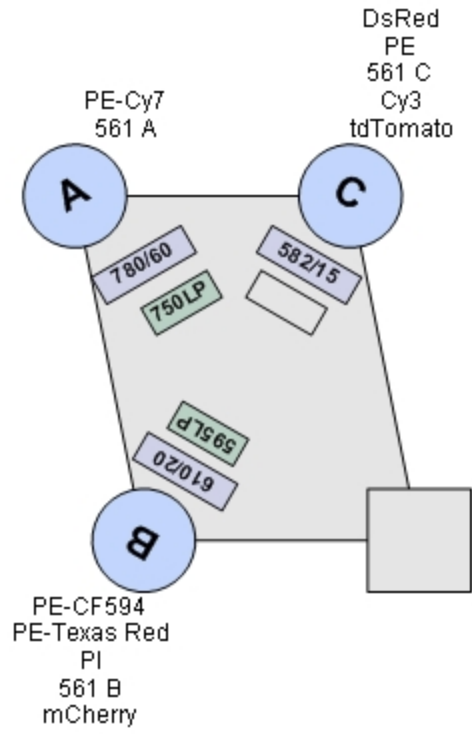

Comments: