



Symphony R0218 Standard Configuration


Cytometer:	LSRFortessa	User:	corestaff
Cytometer Name:	A3 Lite	Institution:	N/A
Serial Number:	R66093700218	Software:	BD FACSDiva 9.3
Input Device:	Manual	Date:	3/2/2023 10:21:37 AM
Window Extension:	10.00		

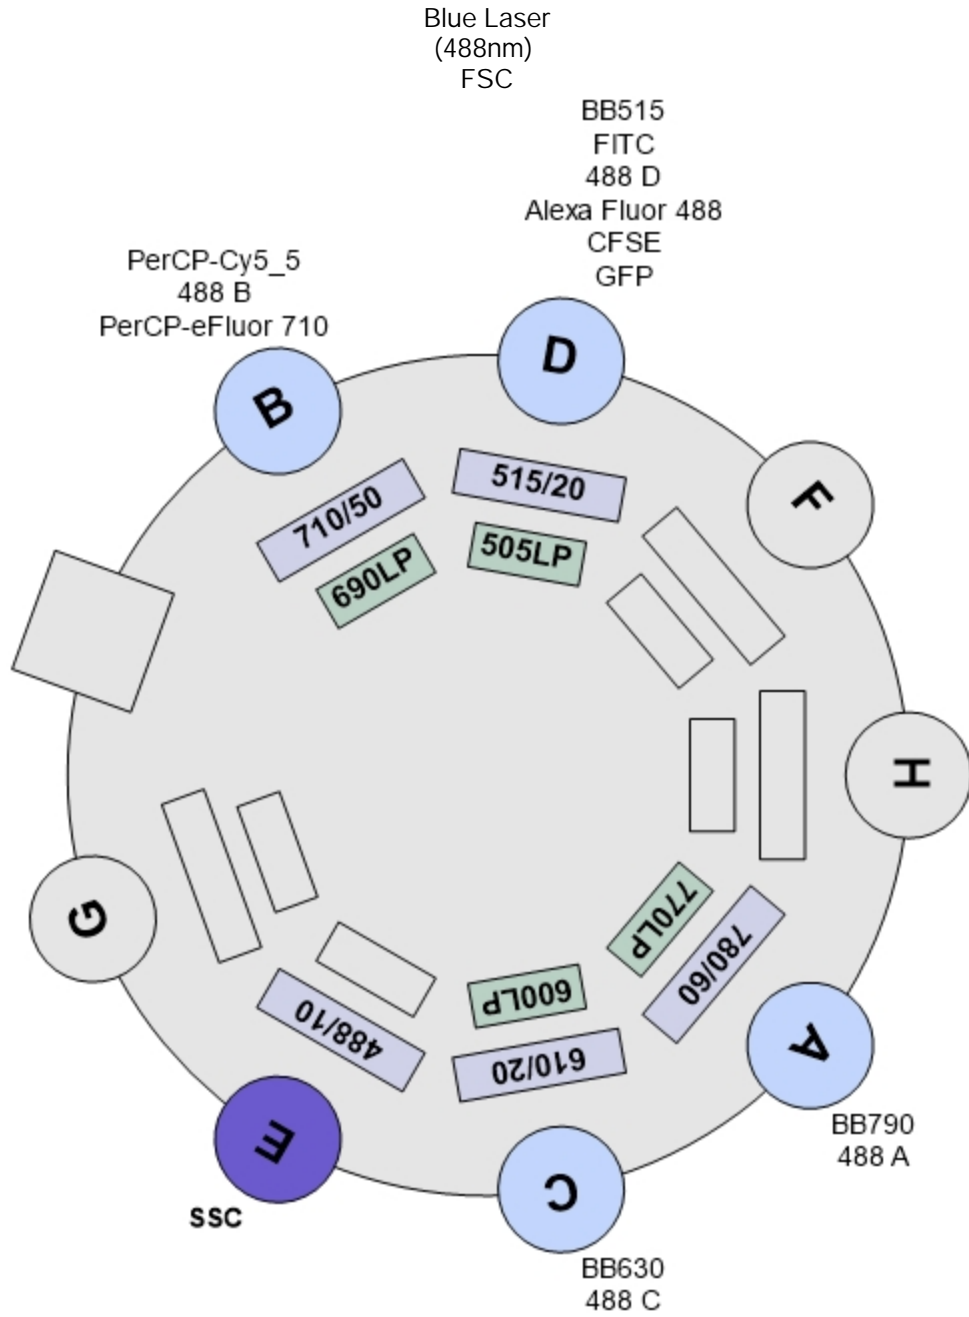


Red Laser
(637nm)

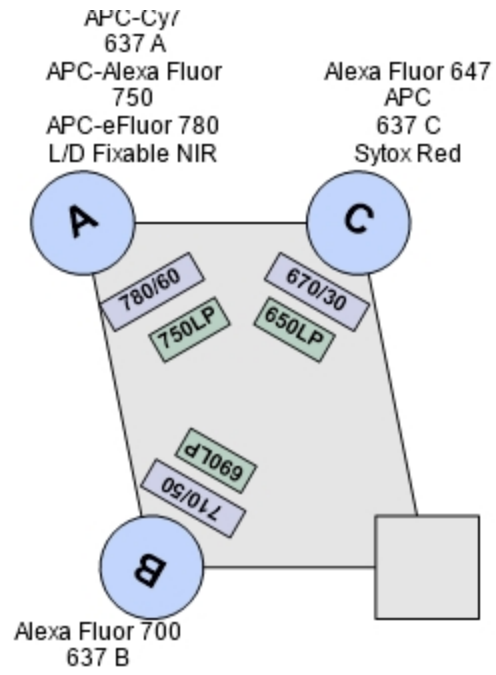


Violet Laser
(405nm)

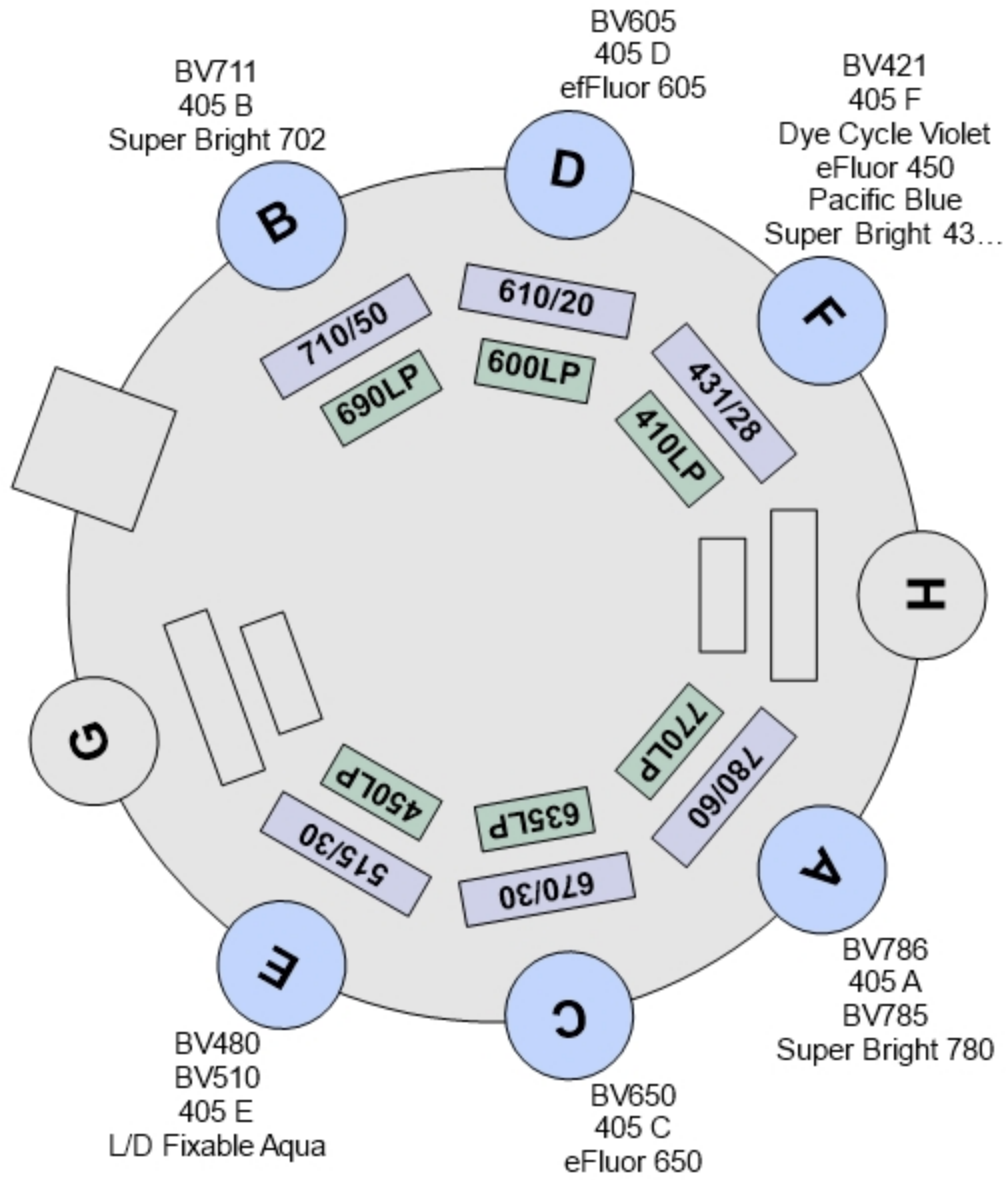

UV Laser
(355nm)

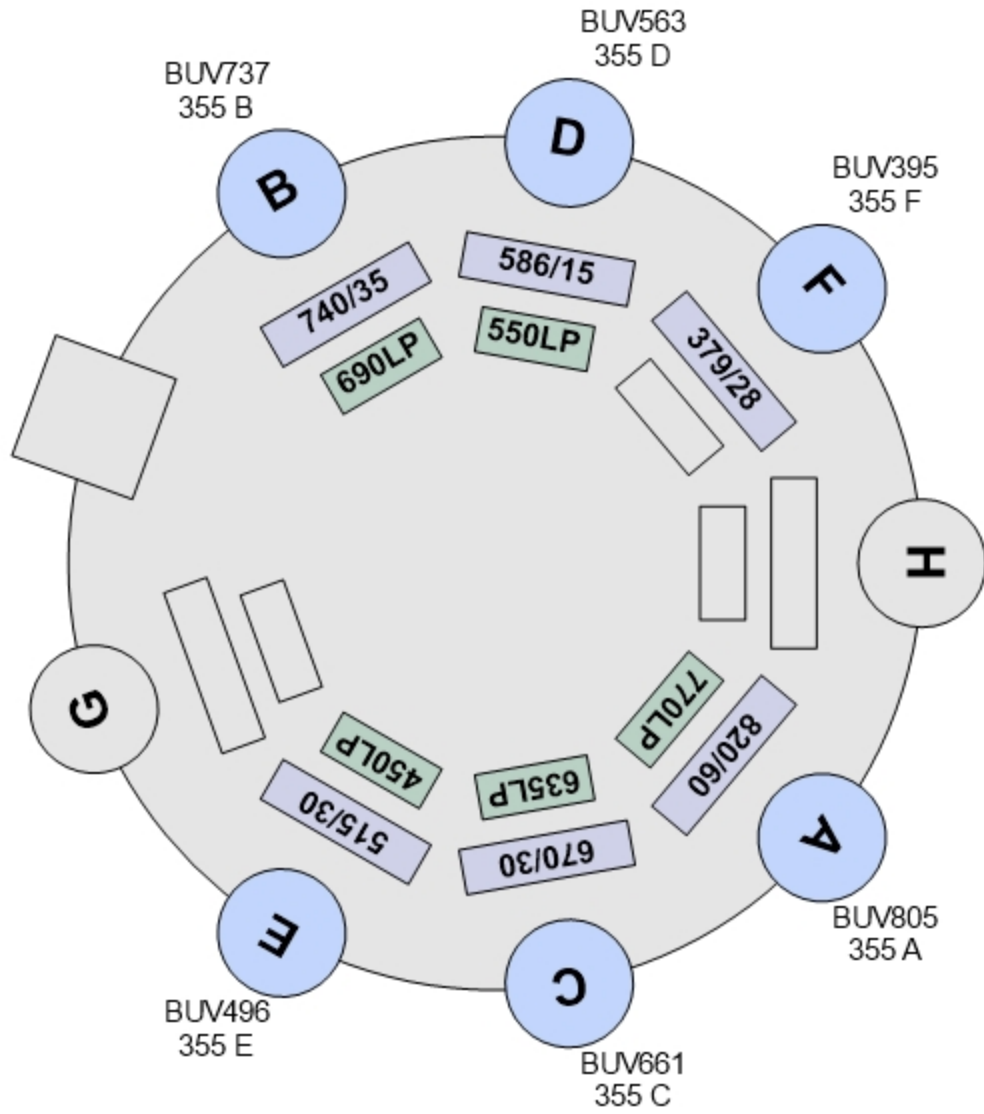

Yellow-Green Laser
(561nm)

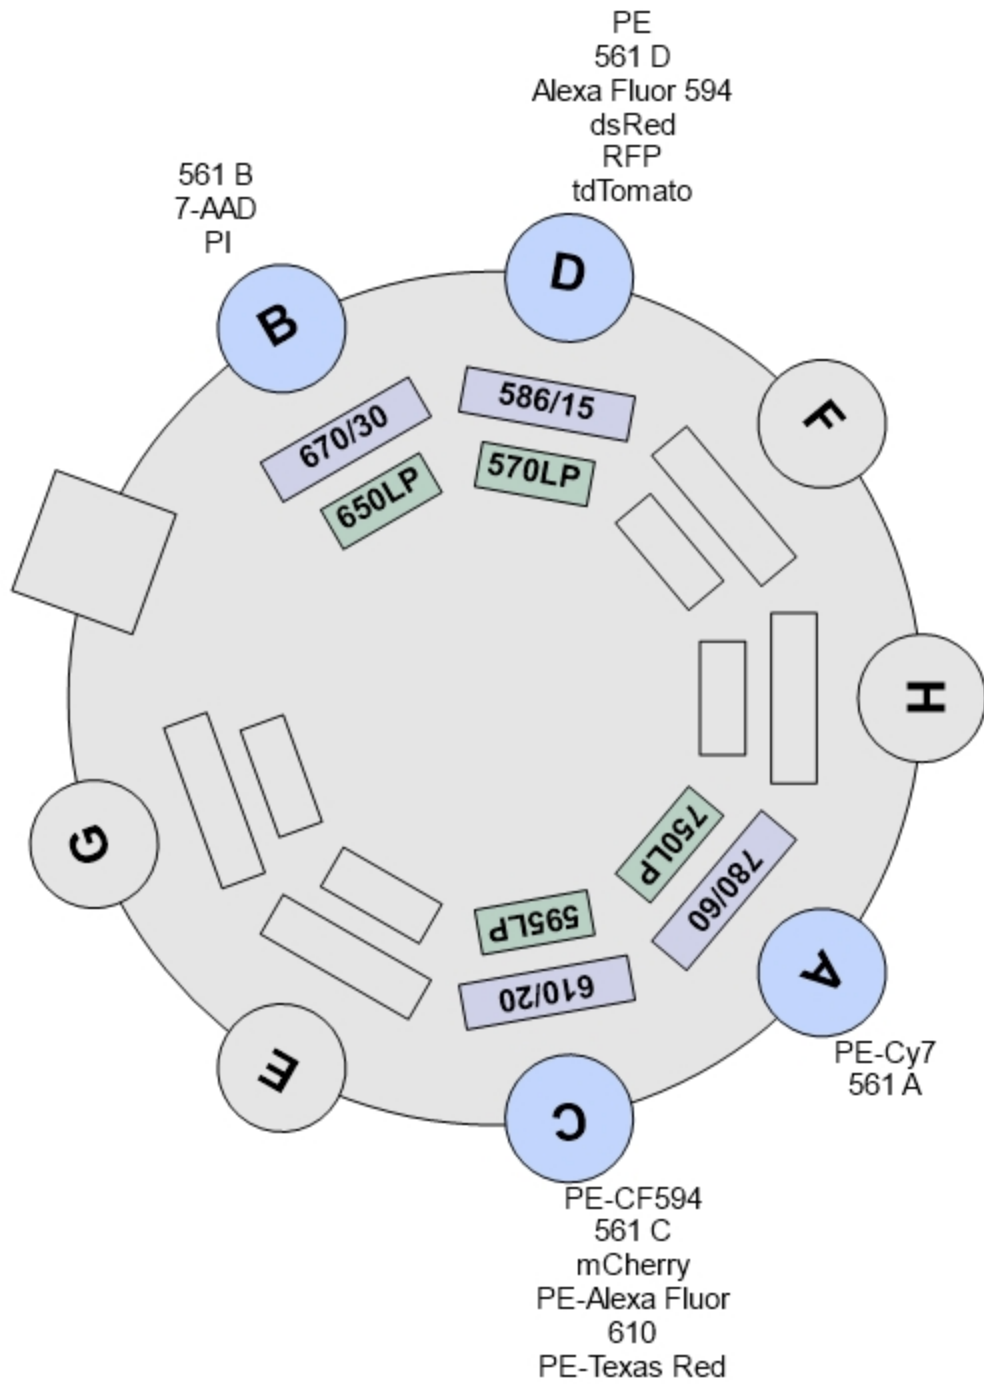

Comments: